

2025 RELEASE UNDER E.O. 14176

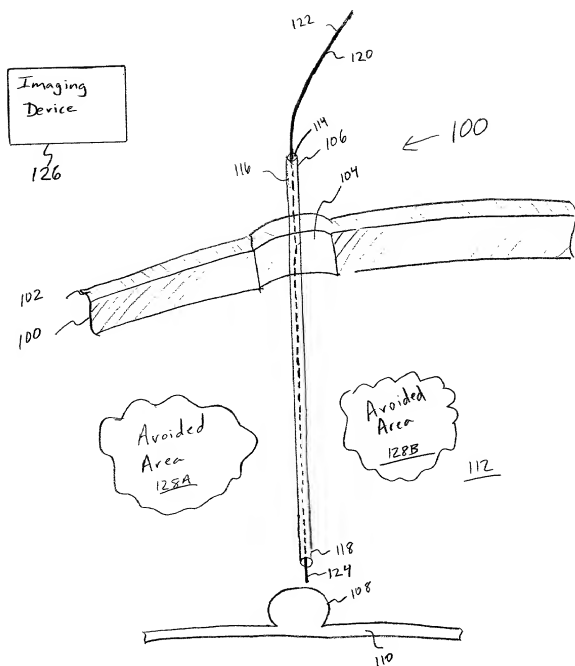


FIG. 1

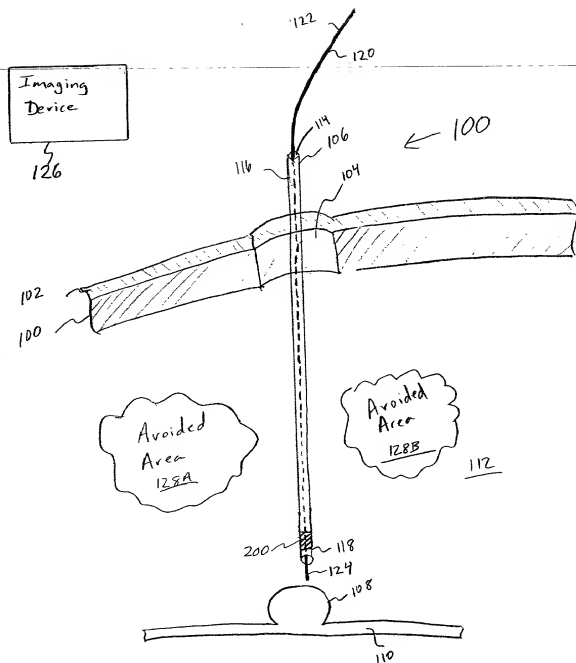


FIG. 2

Imaging
Device

126

122

120

← 100

302

114

106

300

104

102

100

Avoided
Area
128A

Avoided
Area
128B

112


118

124


108

110


FIG. 3

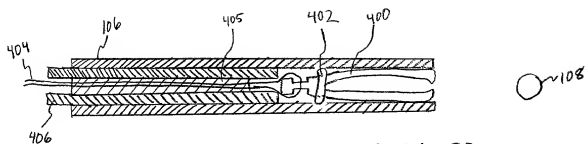


(A) CLIP CLOSED AND RETRACTED

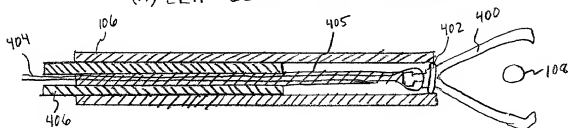

(B) CLIP OPEN AND EXTENDED

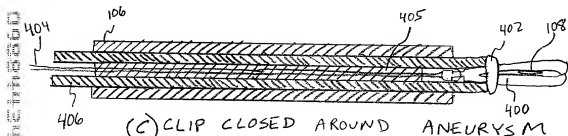

(C) CLIP CLOSED AROUND ANEURYSM



(D) RETAINER OPENED TO RELEASE CLIP

FIG. 5

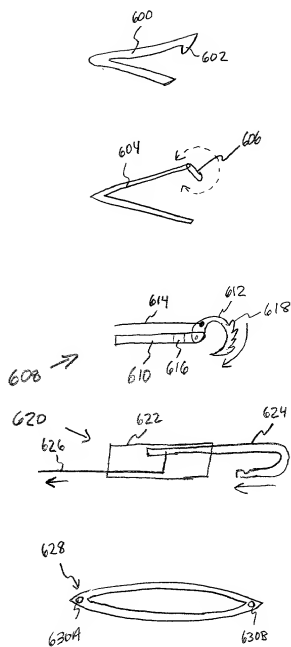


FIG. 6

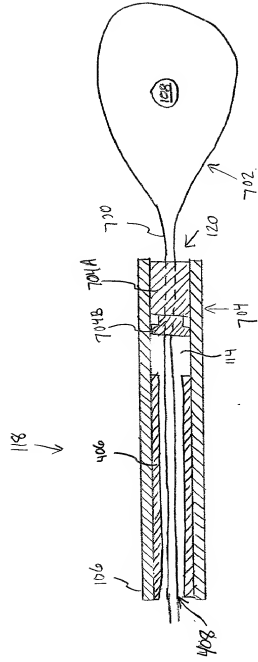


FIG. 7

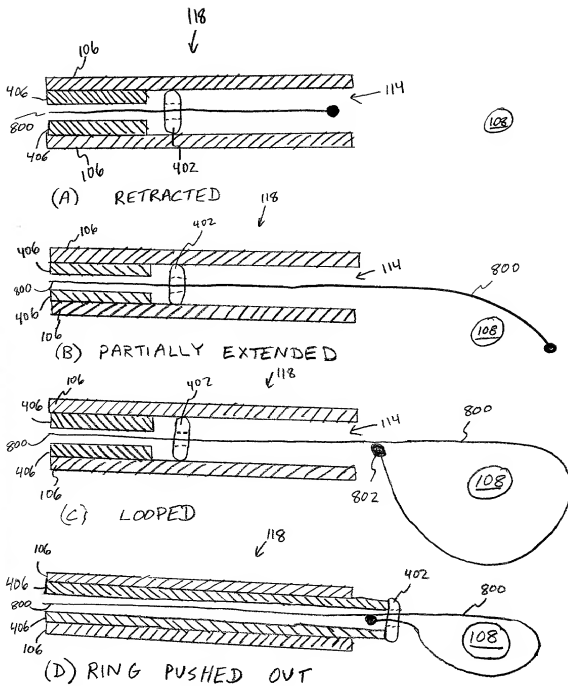


FIG. 8

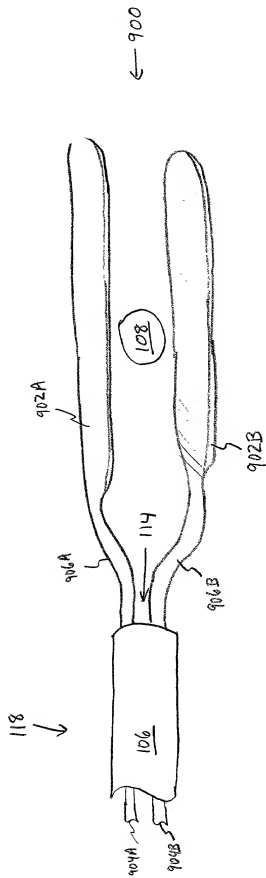


FIG. 9

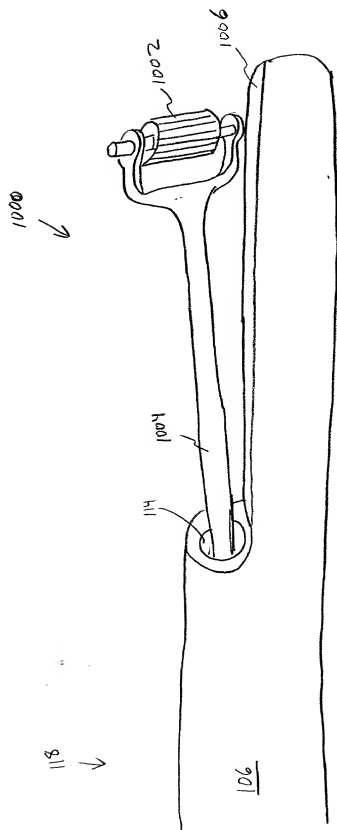


FIG. 10

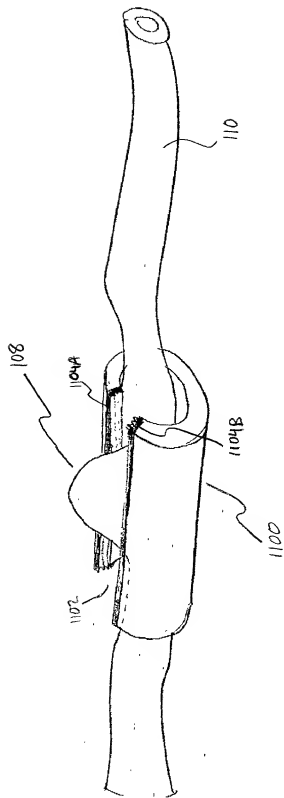


FIG. 11

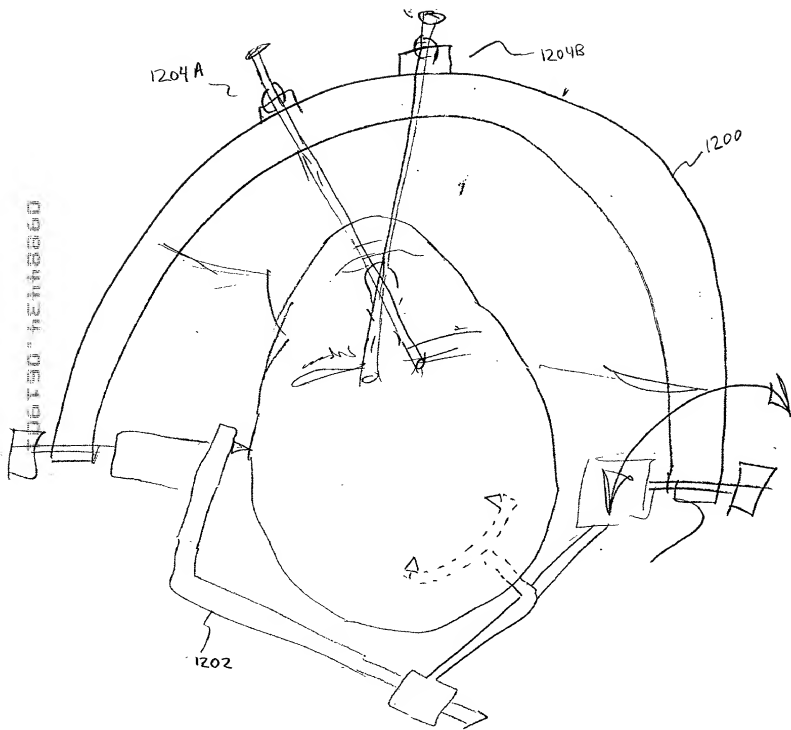


FIG. 12